

عنوان آزمایش : LH-CLIA

عنوان دستگاه : abbot سری ساخت : 33402201

عنوان کنترل : abbot-1

شروع کنترل : 1400/02/01


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
4.471	4.341	4.211	4.081	3.951	3.821	3.691	0.13	3.181

تاریخ	مقدار
22/04/1400	4.32
23/04/1400	4.2
24/04/1400	4.3
26/04/1400	4.3
27/04/1400	4
28/04/1400	4.08

تاریخ	مقدار
12/04/1400	3.9
13/04/1400	4.1
14/04/1400	4.3
15/04/1400	4.09
16/04/1400	4.3
17/04/1400	4.2
19/04/1400	4.3
20/04/1400	4
21/04/1400	4.32

تاریخ	مقدار
01/04/1400	4.3
02/04/1400	3.93
03/04/1400	3.95
05/04/1400	3.9
06/04/1400	4.3
07/04/1400	4.33
08/04/1400	4.13
09/04/1400	3.9
10/04/1400	3.89

Mean: 4.139	SD: 0.168	CV%: 4.061
-------------	-----------	------------

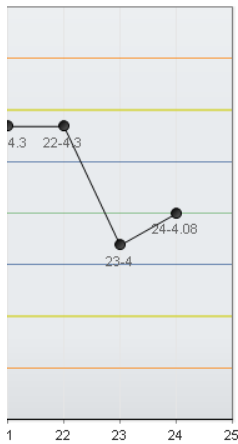



V% 3.181 SD 0.13 -3SD 3.691 -2SD 3.821 -1SD 3.951 Mean 4.081 1SD 4.211 2SD 4.341 3SD 4.471 چاپ

abbott

