

عنوان آزمایش : Progesterone CLIA  
عنوان دستگاه : ABBOTT

سری ساخت : 33402201

عنوان کنترل : ABBOTT-1  
شروع کنترل : 1400/02/01


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
1.114	1.066	1.018	0.97	0.922	0.874	0.826	0.048	4.975

تاریخ	مقدار
22/04/1400	1
23/04/1400	1
24/04/1400	1.06
26/04/1400	1
27/04/1400	1.03
28/04/1400	1

تاریخ	مقدار
12/04/1400	1
13/04/1400	1.05
14/04/1400	1
15/04/1400	1.04
16/04/1400	1.06
17/04/1400	1.05
19/04/1400	1
20/04/1400	0.95
21/04/1400	1.05

تاریخ	مقدار
01/04/1400	1
02/04/1400	1.05
03/04/1400	1
05/04/1400	1
06/04/1400	0.95
07/04/1400	1
08/04/1400	0.95
09/04/1400	1
10/04/1400	0.98

Mean: 1.009	SD: 0.033	CV%: 3.305
-------------	-----------	------------

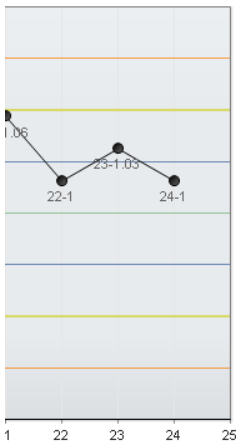

ABBOTT

