

عنوان آزمایش : Triiodothyronine (T3)
عنوان دستگاه : siemens

سری ساخت : 40382

عنوان کنترل : biord II
شروع کنترل : 1399/05/23


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
247.104	233.625	220.146	206.667	193.188	179.709	166.23	13.479	6.522

تاریخ	مقدار
22/04/1400	211
23/04/1400	182
24/04/1400	200
26/04/1400	206
27/04/1400	196
28/04/1400	203
29/04/1400	218
31/04/1400	197

تاریخ	مقدار
12/04/1400	204
13/04/1400	222
14/04/1400	200
15/04/1400	202
16/04/1400	220
17/04/1400	229
19/04/1400	213
20/04/1400	204
21/04/1400	192

تاریخ	مقدار
01/04/1400	188
02/04/1400	194
03/04/1400	196
05/04/1400	214
06/04/1400	211
07/04/1400	209
08/04/1400	219
09/04/1400	226
10/04/1400	216

Mean: 206.615	SD: 11.97	CV%: 5.793
---------------	-----------	------------

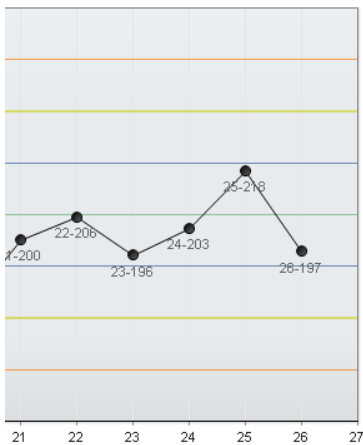

% 6.522 SD 13.479 -3SD 166.23 -2SD 179.709 -1SD 193.188 Mean 206.667 1SD 220.146 2SD 233.625 3SD 247.104

چاپ 🖨

siemens

