

عنوان آزمایش : TPO Ab (Microsomal Ab)-CLIA
عنوان دستگاه : abbot

سری ساخت : 934201

عنوان کنترل : abbot-2
شروع کنترل : 1400/02/04


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
99.243	92.341	85.439	78.537	71.635	64.733	57.831	6.902	8.788

تاریخ	مقدار
22/04/1400	89
23/04/1400	85
24/04/1400	89
26/04/1400	92
27/04/1400	91
28/04/1400	85
31/04/1400	71

تاریخ	مقدار
12/04/1400	79.3
13/04/1400	76
14/04/1400	75.6
15/04/1400	74.6
16/04/1400	80
17/04/1400	85
19/04/1400	82
20/04/1400	83
21/04/1400	76

تاریخ	مقدار
02/04/1400	87
02/04/1400	85
03/04/1400	92
05/04/1400	85
06/04/1400	92
07/04/1400	90
08/04/1400	84
09/04/1400	90
10/04/1400	78

Mean: 83.86	SD: 6.163	CV%: 7.349
-------------	-----------	------------

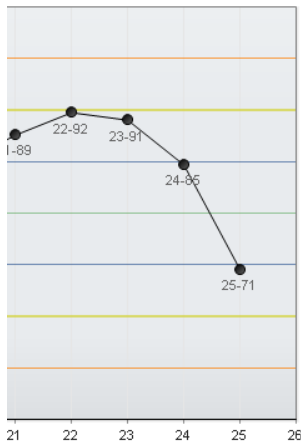



CV% 8.788 SD 6.902 -3SD 57.831 -2SD 64.733 -1SD 71.635 Mean 78.537 1SD 85.439 2SD 92.341 3SD 99.243

چاپ

