

عنوان آزمایش : TSH  
عنوان دستگاه : simense      -سری ساخت : 40382

عنوان کنترل : biorad II  
شروع کنترل : 1399/10/15


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
6.58	6.298	6.016	5.734	5.452	5.17	4.888	0.282	4.912

تاریخ	مقدار
22/04/1400	5.76
23/04/1400	5.17
24/04/1400	5.38
26/04/1400	5.98
27/04/1400	5.21
28/04/1400	5.02
29/04/1400	5.99
31/04/1400	5.71

تاریخ	مقدار
12/04/1400	6.13
13/04/1400	5.04
14/04/1400	5.66
15/04/1400	5.35
16/04/1400	5.38
17/04/1400	5.69
19/04/1400	6.24
20/04/1400	5.47
21/04/1400	5.68

تاریخ	مقدار
01/04/1400	5.27
02/04/1400	5.68
03/04/1400	5.37
05/04/1400	5.47
06/04/1400	5.48
07/04/1400	5.37
08/04/1400	5.21
09/04/1400	5.64
10/04/1400	5.61

Mean: 5.537	SD: 0.317	CV%: 5.721
-------------	-----------	------------

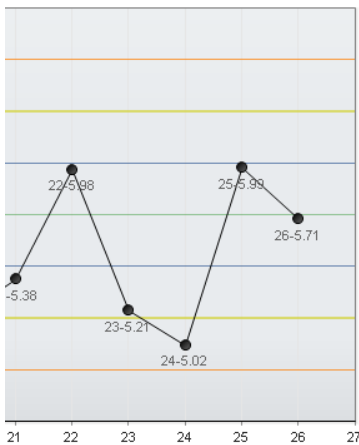



CV% 4.912 SD 0.282 -3SD 4.888 -2SD 5.17 -1SD 5.452 Mean 5.734 1SD 6.016 2SD 6.298 3SD 6.58 چاپ

simense

