

عنوان آزمایش : Testosterone-CLIA
عنوان دستگاه : ABBOT

سری ساخت : 33402201

عنوان کنترل : ABBOTT-1
شروع کنترل : 1400/02/01


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
25.211	23.763	22.315	20.867	19.419	17.971	16.523	1.448	6.937

تاریخ	مقدار
22/04/1400	22.5
23/04/1400	19.4
24/04/1400	22.2
26/04/1400	18
27/04/1400	17
28/04/1400	20.3

تاریخ	مقدار
12/04/1400	21.8
13/04/1400	21
14/04/1400	22.3
15/04/1400	21.8
16/04/1400	22.2
17/04/1400	19.5
19/04/1400	22
20/04/1400	21
21/04/1400	20.8

تاریخ	مقدار
01/04/1400	22.4
02/04/1400	22.3
03/04/1400	21.5
05/04/1400	21
06/04/1400	23
07/04/1400	19.9
08/04/1400	20
09/04/1400	20.5
10/04/1400	21.6

Mean: 21	SD: 1.477	CV%: 7.032
----------	-----------	------------

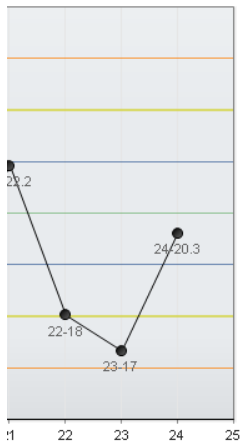



V% 6.937 SD 1.448 -3SD 16.523 -2SD 17.971 -1SD 19.419 Mean 20.867 1SD 22.315 2SD 23.763 3SD 25.211

جاب

ABBOT

